


## Example of kb3.02 – Human weight support

pd specs for an operator seat: as mi01(lower legs and feet), mi03(pelvic area), mi02(thigh), mi04(upper trunk), mi05(head) and mi07(upper arms and elbows), mi08(forearms and wrists). The mi03,02 specs are most detailed. Mi03,02 needs reasons for specs of 7 sections related to the rotation axis of the seat as shown below.

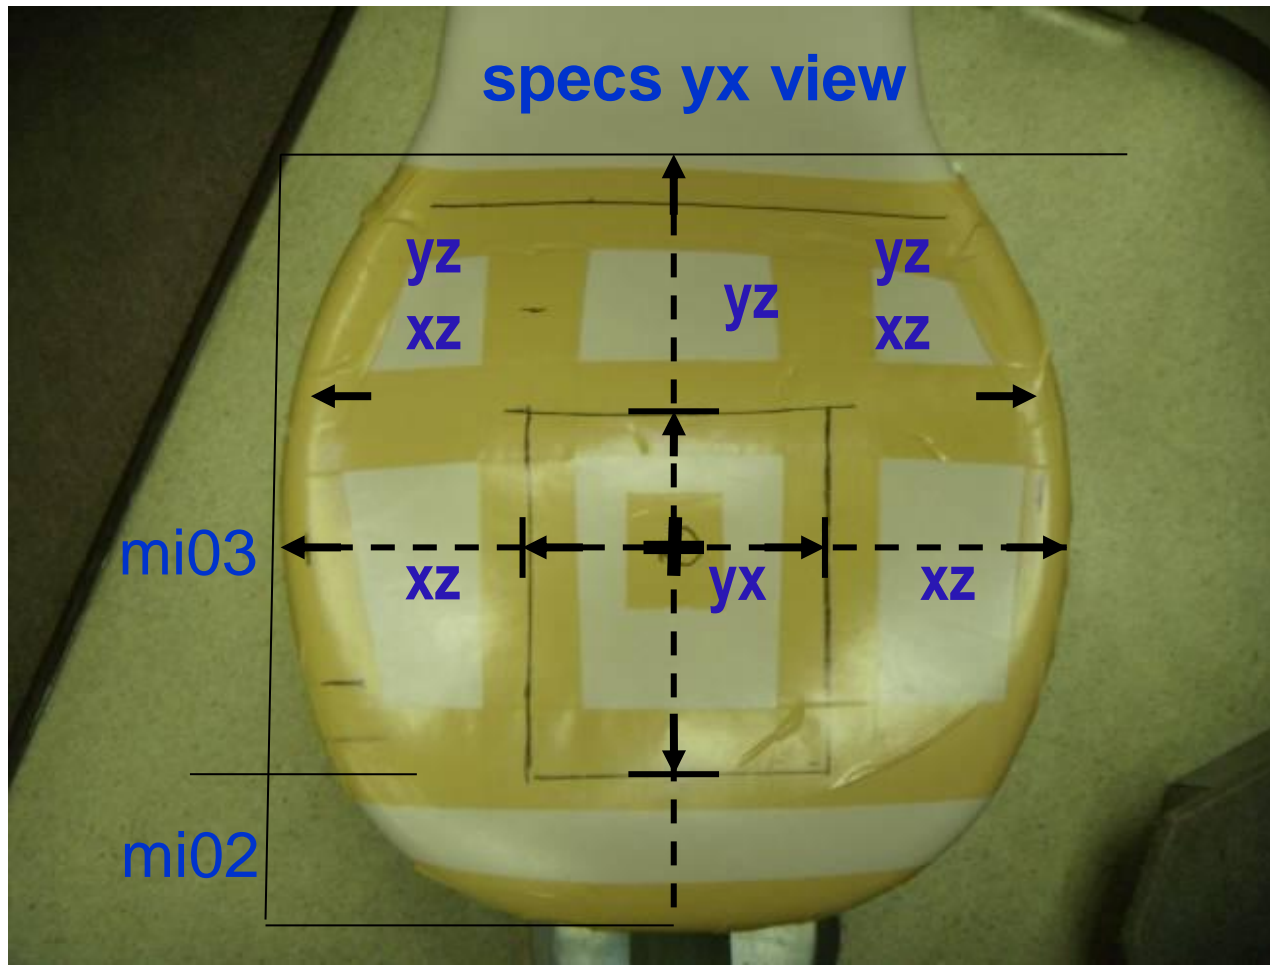

**mi04, 07, 08 contacts are unacceptable (3).**

**mi03 is not recommended (2). (accepted for disabled backs)**

**mi01 use with wheels are not recommended (2).**

**Bars that restrict foot movement are unacceptable (3).**

**A well-installed pivot rotation and seat slide can approach reference (0) or acceptable (1) ratings.**

### **GEPEC pd Ratings**

- 0 Reference**
- 1 Acceptable**
- 2 Not Recommended**
- 3 Unacceptable**